


PRODUCT TECHNICAL DATASHEET

ITEM REF: 011-H1268 REVISION: 19

icumedical
human connections

LEGAL MANUFACTURER	ICU Medical, Inc. 951 Calle Amanecer, San Clemente, CA 92673, USA						
IMPORTER	ICU Medical B.V. Hofspoor 3, 3994 VZ Houten, The Netherlands						
EU AUTHORISED REPRESENTATIVE (EUAR)	Medical Device Safety Service GmbH (MDSS), Schiffgraben 41, 30175 Hannover, Germany						
ASSEMBLY SITE	ICU Medical de Mexico, S.A. de C., Avenida Cuarza No. 250, Colonia Rancho Santa Clara, Delegacion Manadero Ensenada, Baja California, Mexico 22790						
CLASSIFICATION CODE	GMDN Code: 58977						
INTENDED USE	<p>Basic intravenous administration set</p> <p>A collection of sterile devices designed to conduct fluids from an intravenous (IV) fluid container to a patient's venous system. It typically includes tubing, connectors, chambers, clamps, and needles or injection ports. It is typically used for gravitational intravenous administration. This is a single-use device.</p>						
ITEM DESCRIPTION	30 cm (12") Appx 3.2 mL, Set per Infusione, 4 Clave® Connector, Filtro						
PRIMING VOLUME (ml)	3.2	LENGTH (cm)	30,48	WEIGHT (g)	23.53	CASE QTY	50

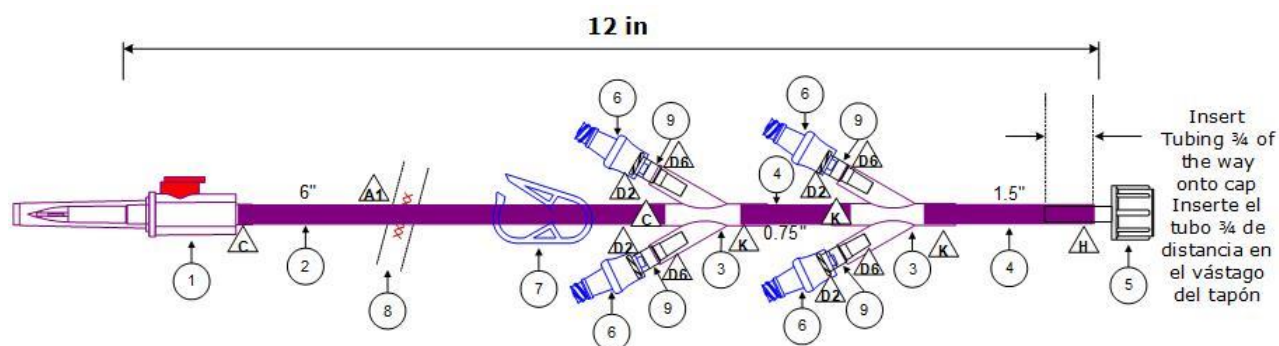

Please don't change tubing Lengths per Customer Request /
Favor de no cambiar las medidas del tubo por requerimiento de cliente.

ITEM SPECIFIC DATA	MRI Compatibility	No metal components
	Chemical Compatibility	Lipids & Common Chemotherapeutics
	Luer Compatibility	ISO 80369-7 Compliant.
	Sterilization and Shelf Life	Radiation; 5-Year Expiration
CLAVE SPECIFIC DATA	Backpressure Rating	60 psig / 3103 mmHG (Activated)
	Disinfection Compatibility	70% Isopropyl Alcohol
	Luer Compatibility	ISO 80369-7 Compliant male luers > 1,55mm Internal diameter
	Backpressure Rating	60 psig / 3103 mmHG (Activated)

PRODUCT TECHNICAL DATASHEET

ITEM REF:

011-H1268

REVISION:

19



LIST OF COMPONENTS <i>(Latex and DEHP Free)</i>	1	SPIKE, BAG, VENTED RED, TUBING	POLYETHYLENE ABS POLYPROPYLENE HYDROPHOBIC AND HAEMOREPELLENT 1.2 MICRON PVDF FORTEX MEMBRANE
	2	TUBING, NATURAL PUR,	POLYURETHANE
	3	CONNECTOR, TRIFURCATED	PVC
	4	TUBING, CLEAR PVC, NO	PVC
	5	CAP, VENTED	HDPE
	6	SUB ASSY, CLAVE WHITE SPIKE	PVC
	7	CLAMP, PINCH, BLUE	POLYPROPYLENE
	8	BANDING TAPE, WHITE W/RED TEXT	TAPE
	9	ADAPTOR, FLL, NO WINGS	PVC
MATERIAL COMPLIANCE AND BIOCOMPATIBILITY	Product has met the requirements of ISO 10993-1 and related standards for biocompatibility.		
PRECAUTIONS	Use aseptic techniques. Single-use only – Do not resterilize. Sterile, Non-Pyrogenic fluid pathway in unopened, undamaged package.		
LABELS AND DIRECTIONS FOR USE	Label and/or DFU contain information for proper use including any warnings or contraindications. Labels are applied on the individual package and on the outside of the cardboard box. Each sales package contains a Direction for Use where applicable.		
PACKING AND PACKAGING	The non-unit packaging is biodegradable as defined by Directive 94/62/EC. Packaging met the requirements of BS EN ISO 11607. The packaging for this product is Latex Free. This item is blister packed or pouched individually using medical grade materials.		
TRACEABILITY	Lot number provides full traceability of all components and manufacturing processes.		
STORAGE	Store in a dry and clean place. Product should be retained in packaging until ready for use.		
DISPOSAL	The user must dispose of the device according to hospital disposal policy.		
PRODUCTION AND ENVIRONMENT CONTROLS	<ul style="list-style-type: none"> Product is manufactured in an environmentally controlled room. Floor, surfaces, and environment are monitored according to quality procedures. Each component is inspected during acceptance (example: visual; dimensional; functional) to verify conformity with the requirements according to quality procedures. Production and release specific tests are performed according to quality procedures. Limulus amebocyte lysate (LAL) testing is performed on production samples to verify conformity of the endotoxin charge according to quality procedures. Bioburden tests are performed on production samples to verify conformity of the microbial charge according to quality procedures. 		

PRODUCT TECHNICAL DATASHEET

ITEM REF:	011-H1268	REVISION:	19
-----------	-----------	-----------	----



QUALITY SYSTEM AND PRODUCT CERTIFICATION	Quality System complies to:	ISO 13485:2016
	Product Certification:	The product is manufactured in compliance to Council Directive MDD 93/42/EEC as amended.
	CE Certificate Number:	252.602
	Notified Body:	NSAI National Standards Authority of Ireland.
	MDD Device Classification:	Class IIa